

Reed
151B

Statements

Official Statement of American Thoracic Society
Medical Section of the American Lung Association

Standardization of Spirometry—1987 Update*

Approved by ATS Board of Directors, March 7, 1987.

CONTENTS

I. INTRODUCTION

II. EQUIPMENT RECOMMENDATIONS

- Recommendation—Vital Capacity (VC)
- Recommendation—Forced Vital Capacity (FVC)
- Recommendation—Timed Forced Expiratory Volume (FEV₁)
- Recommendation—FEF_{25-75%}
- Recommendation—Flow (V)
- Recommendation—Forced Expiratory Time (FET)
- Recommendation—Maximal Voluntary Ventilation (MVV)
- General Background—Spirometry Recorders/Displays
- Recommendation—FVC Volume-Time Curves
- Recommendation—FVC Maneuver Time Scale
- Recommendation—Flow-Volume Curves

III. EQUIPMENT VALIDATION

- Recommendation—FVC Validation of Test Equipment

Recommendation—MVV Validation Equipment

IV. EQUIPMENT QUALITY CONTROL

- Recommendation—Equipment Quality Control

V. MANEUVER PERFORMANCE RECOMMENDATIONS

- Personnel Qualifications
- Recommendation—FVC Subject Instruction and Maneuver
- Recommendation—FVC End-of-Test Criteria
- Recommendation—Minimum FVC Exhalation Time
- Recommendation—FVC Satisfactory Start-of-Test Criteria
- Recommendation—FVC Maximum Number of Maneuvers
- Recommendation—FVC Environmental Conditions
- Recommendation—FVC Use of Nose Clips
- Recommendation—FVC Sitting versus Standing

VI. MEASUREMENT PROCEDURES

- Measurement
- Recommendation—Test Result Selection/Reporting of Results

VII. ACCEPTABILITY AND REPRODUCIBILITY

- Recommendation—FVC Maneuver Acceptability
- Recommendation—FVC Test Result Reproducibility

VIII. REFERENCE VALUES AND INTERPRETATION STANDARDIZATION

IX. CLINICAL ASSESSMENT

- Clinical/Epidemiologic Considerations
- Classification

References

- Appendix A—Signal Processing Tutorial
- Appendix B—Standard Waveforms for Spirometer Validation
- Appendix C—Standard Waveforms

*Published concurrently in the American Review of Respiratory Disease (Am Rev Respir Dis 1987;136 [5]). A copy of this Statement is available from state or local American Lung Association offices.

I. INTRODUCTION

The American Thoracic Society (ATS) Statement on the Standardization of Spirometry was published in 1979 and was based on the Snowbird Workshop held in 1977 [1]. Since that time we have had years of practical experience with these recommendations, which have been widely endorsed [2-5]. In addition, the 'state of the art' of spirometry has advanced as a result of scientific studies that have provided additional data relating to performance of spirometry. Simultaneously the use of computers for spirometry measurement has become commonplace. As a consequence, the American Thoracic Society's Board of Directors asked that the Committee on Proficiency Standards for Clinical Pulmonary Function Laboratories review and update the initial statement.

The ATS statement on standardization of spirometry has had a far-reaching effect on manufacturers and users of spirometers. In some cases, manufacturers have used the document as a 'minimum' performance-requirements document. We are concerned about this approach and encourage manufacturers to continue to seek excellence in design so that the state of the art for spirometers will *exceed* the ATS recommendations. Some research protocols will necessitate even more stringent requirements than those stated here.

We frequently hear the appeal that an inexpensive and, although not explicitly stated, "less-accurate" spirometer is all that is needed in clinical practice. We feel this premise is flawed because treatment decisions need to be based on the best data available, whether data arise from a hospital-based diagnostic laboratory or a physician's office. During recent testing of commercially available spirometers, devices were found that had FVC errors as large as 1.5 liters, a 25% error [6]. If a bronchodilator treatment is given based on spirometric data, subsequent spirometric measurements are often made to determine whether the treatment was effective. If an inaccurate spirometer is used, especially a spirometer with poor repeatability, the improvement or degradation measured may be entirely spirometer-related and have nothing to do with the subject's response to treatment.

Spirometry affects answers to questions about individual patients such as: Does this

subject have enough evidence of impaired lung function to preclude working at a specific job? Should steroid treatment be continued? Does the person qualify for full disability compensation on the basis of impaired lung function? Should the subject's insurance status be changed? Answers to each of these questions based on spirometric maneuvers can have a dramatic effect on a person's lifestyle, standard of living, and future treatment [5].

Similarly, accurate spirometers are required for epidemiologic studies. Rates of improvement or deterioration of pulmonary function measured in relation to environmental exposures and/or personal characteristics may be erroneous if inaccurate spirometers are used or less sensitive if imprecise spirometers are used [7].

Testing of commercially available spirometers, with a computer-driven mechanical syringe, has recently been completed. It was found that already 27 of 53 (51%) spirometers met the new and rigorous ATS recommendations outlined in this document. With the aid of microcomputers, several flowmeter-type spirometers now meet the ATS requirements [6]. Not surprisingly, computer software was one of the major reasons for device failure.

Maximizing the clinical usefulness of spirometry depends upon a number of factors ranging from equipment selection to interpretation and ultimately involves clinical assessment. Figure 1 is a flow diagram of these steps. The first step is choosing the equipment. The Snowbird Workshop [1] and now this update give recommendations for equipment used for spirometry. Spirometer users should carefully select equipment that meets the ATS recommendations to assure that spirometry testing can be done accurately. The second step in the process involves validating that the spirometer design and that a production device meet the recommendations. Detailed methods for performing the validation testing are outlined later in this article. Because almost no physicians and few clinical pulmonary function laboratories have the capability to exhaustively test and validate spirometers, an independent testing laboratory has been set up at LDS Hospital in Salt Lake City, Utah. Other independent laboratories are encouraged to enter the spirometer validation field.

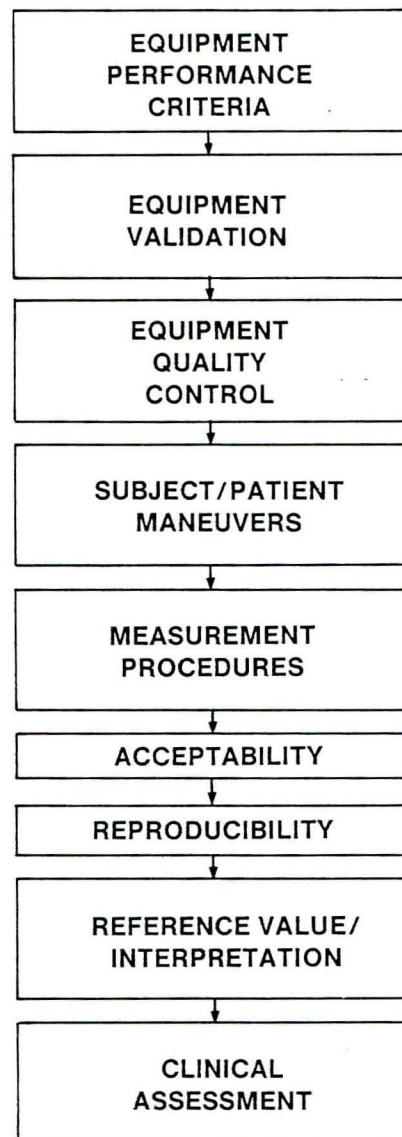


Fig. 1. Spirometry standardization steps.

The ATS promulgates standards but does not act as a certifying agency to verify compliance with these standards. Before a user purchases a spirometer, he or she would be wise to (1) ask the manufacturer to provide summary data that demonstrate that the device being considered meets the ATS recommendations and (2) review results of spirometry testing from independent testing laboratories.

Even after the equipment has been found to meet ATS recommendations and has been validated, spirometers (like other pieces of mechanical, electrical, or computer equipment) must be routinely

checked for performance quality. Recommendations for spirometer quality control have been developed by the ATS and are summarized in this article.

Spirometry is an effort-dependent maneuver that requires careful patient/subject instruction, understanding, coordination, and cooperation. Thus, performance recommendations are important components of testing. Part of the recommendation is to obtain a sufficient number of maneuvers that are of adequate quality and then to determine whether these acceptable maneuvers are reproducible. Once spirometry maneuvers have been performed they need to be measured either by hand or by use of computer techniques. Measurement procedures are included in this article to help assure that uniform methods are used and that comparable results are obtained. These recommendations include considerations such as the use of "back extrapolation" for determining the "start-of-test" time-zero point for determination of measures such as FEV₁.

Interaction between technician and patient or subject is crucial to performing adequate spirometry because it is such an effort-dependent maneuver. Technicians must be selected and trained and must maintain a high level of proficiency to assure optimum results.

The effort-dependent spirogram must be carefully scrutinized for quality. Recommendations about quality, acceptability, and reproducibility of test results are presented. After adequate results are obtained, they are usually compared with reference values to make an assessment (interpretation) of the results. Future ATS efforts should be directed to investigating and providing guidelines for selecting reference values and interpretive methods. This article provides only background materials for these future developments.

Clinical assessment is a crucial part of the patient/subject-physician/investigator interaction and should be an integral part of the entire process. Results obtained from spirometry are only one part of the much more complex patient care relationship of research data analysis.

Definitions

Standard definitions are important to assure that everyone understands each test

and its performance methodology. All terms and abbreviations used here are based on a report of the American College of Chest Physicians (ACCP)-ATS Joint Committee on Pulmonary Nomenclature [8].

II. EQUIPMENT RECOMMENDATIONS

Equipment selection is pivotal to acquiring accurate test results. Spirometer equipment recommendations apply to all diagnostic spirometers whether used for clinical, diagnostic, or epidemiologic purposes. Instrumentation recommendations should be followed to provide accurate spirometric data and information that is comparable from laboratory to laboratory and from one time period to another [1]. The accuracy of a spirometer system depends on the resolution (ie, the minimum detectable volume or flow) and linearity of the entire system—from volume or flow transducer to recorder, display, or processor. Errors at any step in the process affect the accuracy of the results obtained (see Appendix A). For example, if a sample point is not available at exactly 1.0 s after the back extrapolated "time zero," then linear interpolation of the volume curve should be used to find FEV₁.

The equipment recommendations for spirometry are summarized in Table 1.

Recommendation—Vital Capacity (VC)

VC = the maximal volume of air exhaled from the point of maximal inhalation. This is also considered the "slow" vital capacity and is expressed in liters (BTPS). BTPS = body conditions: normal body temperature (37° C), ambient pressure, saturated with water vapor.

Recommendation—VC Equipment

If a spirometer purports to measure VC, it should continue to accumulate volume for **at least** 30 s. Spirometers should be capable of measuring volumes of **at least** 7 L (BTPS) with flows between 0 and 12 L/s. Accuracy required is **at least** $\pm 3\%$ of reading or ± 0.050 L, whichever is greater.

Rationale. Based on Hankinson and Petersen's data on 9,347 working coal miners, the ranges for volume and flow were established [1,9]. Of these miners, 99.25% had a forced vital capacity of less than 7.25 L [1]. If the spirometer is used for both inspiration and expiration, a volume capacity of greater than 7 L may be necessary. The volume requirement of 7 L also applies to children [1,3,10,11]. Older men and women have volumes similar to those of adolescents [10-12]. A 7-L spirometer will not measure the person with 'super' lungs, but it will cover the majority of the population. Accuracy of $\pm 3\%$ of reading or ± 0.050 L, whichever is greater, is based on the data of Hankinson and Petersen [1,9]. Their data showed coefficient of variation of 3% or less on the same subject on different days [1]. These data have been substantiated [13-15]. A spirometer must be capable of measuring flows in the range of 0 to 12 L/s. The 12 L/s maximal flow rate selection was determined from Hankinson and Petersen's data [1,9] that showed that less than about 7% of the miners had flow rates greater than 12 L/s.

Recommendation—Forced Vital Capacity (FVC)

FVC = maximal volume of air exhaled with maximally forced effort from a position of maximal inspiration. Vital capacity is performed with a maximally forced expiratory effort and is expressed in liters (BTPS).

Recommendation—FVC Equipment

The spirometer should be capable of measuring volumes up to **at least** 7 L (BTPS) with an accuracy of **at least** $\pm 3\%$ of reading or ± 0.050 L, whichever is greater, with flows between 0 and 12 L/s. The spirometer should be capable of accumulating volume for **at least** 15 s, although longer times are recommended.

Rationale. Subjects and patients can exhale for longer than 15 s; so, instruments should be capable of measuring their true FVC. For the FVC maneuver, the volume requirements are the same as for the VC [1,9-13]. The spirometer must be capable of measuring flows in the range of 0 to 12 L/s. The 12 L/s maximal flow rate

Table 1. Minimal Recommendations for Spirometry Systems

Test	Range/Accuracy BTPS (L)	Flow Range (L/s)	Time (s)	Resistance and Back Pressure	Test Signal
VC	7 L \pm 3% of reading or \pm 0.005 L, whichever is greater	0 to 12	30		3-L calibrating syringe
FVC	7 L \pm 3% of reading or \pm 0.005 L, whichever is greater	0 to 12	15		24 standard waveforms
FEV ₁	7 L \pm 3% of reading or \pm 0.005 L, whichever is greater	0 to 12	t	Less than 1.5 cm H ₂ O/L/s, from 0 to 12 L/s	24 standard waveforms
Time Zero	The time point from which all FEV ₁ measurements are taken			Determined by back extrapolation	
FEF _{25-75%}	7 L \pm 5% of reading or \pm 0.200 L/s, whichever is greater	0 to 12	15	Same as FEV ₁	24 standard waveforms
\dot{V}	12 L/s \pm 5% of reading or \pm 0.200 L/s, whichever is greater	0 to 12	15	Same as FEV ₁	Manufacturer proof
MVV	Sine wave 250 L/min at V _T of 2 L within \pm 5% of reading	0 to 12 \pm 5%	12 to 15 \pm 3%	Pressure less than \pm 10 cm H ₂ O at 2-L V _T 2.0 Hz	Sine wave pump 0 to 4 Hz \pm 10% at \pm 12 L/s

selection was based on Hankinson and Petersen's data, which showed that fewer than 7% of their coal miners had peak flows greater than 12 L/s [1,9].

Recommendation—Timed Forced Expiratory Volume (FEV_t)

FEV_t = the volume of air exhaled in the specified time during the performance of the FVC, eg, FEV₁ for the volume of air exhaled during the first second of FVC. It is expressed in liters (BTPS).

Recommendation—FEV₁ Equipment

Measuring the FEV₁ requires a spirometer having a volume of *at least* 7 L. The spirometer should measure the FEV₁ within an accuracy of *at least* \pm 3% of reading or \pm 0.050 L, whichever is greater, with flows between 0 and 12 L/s. The "start of test" for purposes of timing *will be* determined by the back-

extrapolation method [1,16,17] or a method shown to be equivalent. (See Figure 2). For hand measurements, the back-extrapolation method traces back from the steepest slope on the volume-time curve (See Figure 2) [17,18]. For purposes of computer methods of back extrapolation, we recommend using the largest average slope over a 70-ms period [19] (Appendix A). The resistance to air flow from 0 to 12 L/s should be less than 1.5 cm H₂O/L/s.

Rationale. FEV₁ measurement is influenced by the point selected as the start of the maneuver. A uniform method of selecting the point is required to maintain consistency. The back-extrapolation [1,16,17] method is the most consistent and accepted method (see Section VI for measurement procedures) and should be used until other methods are demonstrated to give equivalent results. One attempt to demonstrate equivalency of volume- or flow-threshold methods for detection of start of test by back extrapolation was unsuccessful [20]. Resistance to flow affects

the FEV₁ and other timed expirations [21-26].

Recommendation—FEF_{25-75%}

FEF_{25-75%} = mean forced expiratory flow during the middle half of the FVC. Formerly it was called the maximal

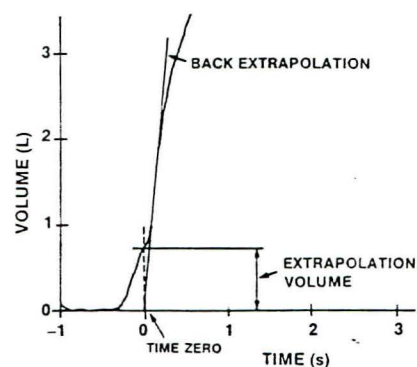


Fig. 2. Typical subject waveform of a volume-time spirogram illustrating back extrapolation to determine "time zero."

midexpiratory flow rate (MMEF) and is expressed in L/s (BTPS).

**Recommendation— $FEF_{25-75\%}$
Equipment**

The $FEF_{25-75\%}$ should be measured with an accuracy of **at least** $\pm 5\%$ of reading or ± 0.200 L/s, whichever is greater. The $FEF_{25-75\%}$ should be measured on a system that meets the FVC recommendations.

Rationale. The $FEF_{25-75\%}$ maneuver has a much larger intra-subject variability than FVC or FEV_1 [27]. Additionally, two measurements of both volume and time are required; therefore, the relaxed accuracy requirement is justified. Manufacturers and software developers should be aware that a major error in $FEF_{25-75\%}$ can occur when slow-sampling-rate analog-to-digital converters are used. With these systems it may be necessary to interpolate between sample points to get the exact 25% and 75% of FVC points.

Recommendation—Flow (\dot{V})

\dot{V} = instantaneous forced expiratory flow and is expressed in L/s (BTPS).

Recommendation—Flow Measurement

Flow may be measured electronically or manually. Where flow-volume loops or other uses of flow are made, with flow in the range of -12 to $+12$ L/s, the flow should be within $\pm 5\%$ of reading or ± 0.200 L/s, whichever is greater.

Rationale. Flow-measuring devices such as pneumotachometers increasingly are being used to measure spirometric parameters [6]. With flow devices, volume is determined by integration of flow. Flow-calibration methods with sufficient accuracy have not yet been developed. Volume spirometers differentiate volume signals to determine flow. With the 'noise,' phase-shift, and associated problems, flows accurate to within $\pm 5\%$ are thought to be adequate. Whenever a flow signal is integrated to measure volume, the volume accuracy requirements are $\pm 3\%$ of reading or ± 0.050 L, whichever is greater [1]. Instantaneous flows parameters such as $FEF_{75\%}$, FEF_{max} , and peak expiratory flow rate (PEFR) are very device-dependent and as a consequence their measurements are quite variable [6].

Recommendation—Forced Expiratory Time (FET)

FET = time from the back extrapolated "time zero" until the first inspiratory effort following FVC or the end of expiratory effort.

Rationale. The FET helps show that the duration of FVC effort was acceptable, an especially useful measure when flow-volume loops are used.

Recommendation—Maximal Voluntary Ventilation (MVV)

MVV = the volume of air exhaled in a specified period during repetitive maximal respiratory effort and is expressed in L/min (BTPS).

Recommendation—MVV Equipment

When a spirometer is used for measuring MVV, it should have an amplitude-frequency response that is flat within $\pm 10\%$ from 0 (DC) to 4 Hz at flow rates of up to 12 L/s over the volume range. The time for exhaled volume integration or recording should be no less than 12 or more than 15 s [21]. The indicated time should be accurate to within $\pm 3\%$.

Rationale. For the MVV maneuver, the frequency content of the volume-time signal is high [28,29]. Results are dependent on the patient effort as well as the frequency response characteristics of the spirometer [21,30-32].

General Background—Spirometry Recorders/Displays

Paper records or graphic displays of spirometry signals are **required** and are used for 3 primary purposes:

(1) *Diagnostic* function—when waveforms are to be used for quality control or review of the forced expiratory maneuver—to determine whether the maneuver was performed properly, so that unacceptable maneuvers can be eliminated.

(2) *Validation* function—when waveforms are to be used to validate the spirometer system hardware and software for accuracy and reliability through the use

of hand measurements (for example, measurement of FEV_1 using back extrapolation by comparing computer- and hand-determined FEV_1).

(3) *Hand measurement* function—when waveforms are to be hand measured for spirometric parameters (FVC, FEV_1 , etc.) in the absence or failure of a computer.

With recent advances in computer technology, there are many different ways to display and record spirometric waveforms. The Committee has chosen to broaden the initial scope of the spirometry standardization document to further encourage use of computer technology.

A less stringent paper recorder requirement will suffice for *diagnostic* purposes compared to *validation* and *hand measurement* needs. If no paper recorder or printer is available or if the paper recorder does not meet the requirements for *validation* and *hand measurement* applications, then proof of validation of the accuracy and stability of the spirometer by an independent laboratory **must** be provided by the manufacturer. For these computer methods, any new software releases **must** also be validated. *Users and manufacturers* should realize that for certain applications (for example, for disability determination and legal cases), diagnostic size displays are **not** adequate [21]. For example, with the Cotton Dust standard "... tracings must be stored and available for recall and must be of sufficient size that hand measurements may be made ..." [33]. Also users will customarily not be able to verify accuracy and stability of spirometers by themselves in the absence of an adequate paper recording.

Recommendation—FVC Volume-Time Curves

When a volume-time curve is plotted or displayed, the volume scale for each of the following conditions should be **at least**

(1) *Diagnostic* function: 5 mm/L (BTPS) for volume so the graphs will be large enough to allow recognition of unacceptable maneuvers and disease patterns.

(2) *Validation* and *hand measurement* functions: 10 mm/L (BTPS) for volume for validation and measurement functions. See section below for time scale of volume-time plots.

Recommendation—FVC Maneuver Time Scale

(1) *Diagnostic* function: time scale, **at least** 1 cm/s.

(2) *Validation* and *hand measurement* functions: time scale, **at least** 2 cm/s; when hand measurements are made, larger time scales are preferred (at least 3 cm/s) but are not required [1,34,35].

Rationale. A recent study [35] evaluating the effects of time scale (paper speed) on spirometry accuracy has recommended a time scale of at least 3 cm/s if spirometry are to be accurately measured by hand. This more stringent criterion was considered, but not adopted as a minimum recommendation. The new study further supports the current 2 cm/s requirement as a minimum recommendation [35]. Because so many spirometers now make use of computers, time resolution and sampling rate become important design issues. The tutorial in Appendix A and Table 2 give further specification details.

Recommendation—Flow-Volume Curves

When a flow-volume curve is plotted or displayed, exhaled flow should be plotted upwards, and exhaled volume towards the right. A 2:1 ratio should be maintained between the flow and volume scales; eg, 2 L/s of flow and 1 L of exhaled; volume should be the same distance on their respective axes. The minimum flow and volume scales should be **at least** as shown in Table 2:

Rationale. Currently, flow-volume curves are displayed with a variety of orientations

and aspect ratios, hindering the usefulness of visual pattern recognition. Also, some current digitally generated curves do not have sufficient flow or volume resolution. Manufacturers and users should be aware of these limitations.

III. EQUIPMENT VALIDATION

Recommendation—FVC Validation of Test Equipment

The diversity of FVC maneuvers encountered in clinical practice is currently best simulated by the use of the 24 standard waveforms developed by Hankinson and Gardner [19,36]. These waveforms can be used to drive a computer-controlled mechanical syringe for testing actual hardware and software, [6,37] or they can be put into a system in digital form to evaluate **only** the software. Appendix C shows a volume-time and a flow-volume plot of each of the 24 standard waveforms and includes Table 4, which gives the measured values. The American Thoracic Society also provides these waveforms on floppy disks for an IBM PC. Appropriate corrections for using gas at ambient temperature and humidity instead of BTPS may need to be made for some mechanical syringe-spirometer combinations.

The validation limits for volume are: Volume (FVC, FEV₁) ± 3.5% of reading or ± 0.070 L, whichever is greater, and flow (FEF_{25-75%}) ± 5.5% of reading or ± 0.250 L/s, whichever is greater. The error range was expanded from the ATS spirometry recommendation stated earlier to allow for errors associated with mechanical syringes [6]. Mechanical syringes used

for validation must be accurate within ± 0.025 L for FVC and FEV₁ and ± 0.100 L/s for FEF_{25-75%}.

Rationale. Since the publication of the ATS Spirometry Statement, additional efforts by the Association for the Advancement of Medical Instrumentation (AAMI) [36] have resulted in the development of 24 standard waveforms for spirometer evaluation [19]. Because these waveforms were obtained from recordings of actual subject waveforms and have been accepted by AAMI, and because better standard signals are not available, the ATS recommends their use as a test signal for FVC for evaluation of software or entire spirometry systems. When one is evaluating spirometers in which the 24 standard waveform sets are injected from a computer-controlled mechanical syringe [6,37], the spirometer will qualify as meeting ATS requirements if fewer than 1 in every 20 measured values is outside the limits, provided the failure does not represent an inherent design defect.

Flows cannot be generated easily without noise; therefore the frequency of the noise should be stated. In addition, a step-function signal should be generated with the mechanical syringe, and the resulting signal should be sampled at a frequency of at least 1,000 Hz to determine the dynamic characteristics of the driving syringe. Typically, these systems have second-order oscillatory characteristics. By using the step-function signal, the natural frequency and damping coefficients can be determined. Some spirometer manufacturers have appropriately purchased a computer-based syringe system for dynamic testing of each of their own spirometers (MH Custom Design and Manufacturing, 70 Fern Drive, Midvale UT 84047); however, spirometry system designs and a production model must be validated by an independent testing laboratory.

Recommendation—MVV Validation Equipment

When tested with a pump producing a sinusoidal waveform, the indicated response of the spirometer in incrementally increased flows up to 250 L/min signal, produced with stroke volumes up to 2 L, should be accurate within ± 5% of reading.

Table 2. Summary Table of Minimum Required Scale Factors for Time, Volume & Flow Graphics

Variable	Diagnostic Measures		Validation and Measurement	
	Resolution Required	Scale Factor	Resolution Required	Scale Factor
Volume	0.050 L	5 mm/L	0.025 L	10 mm/L
Flow	0.20 L/s	2.5 mm/L/s	0.10 L/s	5 mm/L/s
Time	20 ms	1 (cm/s)	20 ms	2 cm/s

During the testing, the pressure at the mouthpiece should not exceed ± 10 cm H₂O. For volume spirometers, these requirements apply throughout their volume range.

IV. EQUIPMENT QUALITY CONTROL

Routine equipment preventive maintenance, cleaning, calibration checks, verification, and quality control are important to assure accurate spirometry results [38]. A spirometry procedure manual is an important base for a quality assurance program. The manual should contain a quality control plan, guidelines for ordering spirometry, guidelines for performing spirometry, and guidelines for reporting spirometry results. See the document "ATS Quality Assurance for Pulmonary Laboratories" for more details [38].

The role of spirometric equipment in the transmission of infections has not been established [39]. However, general suggestions based on a reasonable theoretical rationale or data from other sources are appropriate. A recent publication by the Centers for Disease Control outlines 9 recommendations: (1) handwashing indications, (2) handwashing technique, (3) handwashing products, (4) handwashing facilities, (5) fluids and medications, (6) handling blood specimens, (7) maintenance of equipment, (8) protection of patients from other infected/colonized patients or staff, and (9) microbiologic monitoring [39].

Recommendation—Equipment Quality Control

The spirometer's ability to accurately measure volume should be checked *at least* daily with a calibrated syringe with a volume of at least 3 L. During industrial surveys or other field studies in which a large number of subject maneuvers are done, the equipment should be calibrated prior to testing daily if in regular use and then every 4 h during use [38]. Although there is minimal day-to-day variation in volume calibration, daily calibration checking is highly recommended so that the onset of a problem can be determined within 1 day, eliminating needless reporting of false values for several weeks or months,

and also to help define day-to-day laboratory variability. For survey testing in which a large number of maneuvers are done, the 4-h period of calibration checking is recommended to prevent invalidation of data from a large number of maneuvers. Spirometer systems should be evaluated for leaks on a daily basis [17,40]. The Intermountain Thoracic Society Manual suggests that leaks be detected by applying a constant positive pressure of 3 cm H₂O or more with the volume spirometer outlet occluded. Any observed volume change after 1 min is indicative of a leak [17]. *at least*, quarterly, volume spirometers should have their calibration checked over their entire volume range (in 1-L increments) using a calibrated 3-L syringe [6]. Two emptying times for the 3-L syringe are indicated; 0.5 to 1 s (flow in the range of 3 to 6 L/s) and, at least, 6 s (flows less than 0.5 L/s). Assessing the recorder time-scale accuracy with a stopwatch should be performed *at least* quarterly. An accuracy of within 1% should be achieved. If equipment is changed or relocated (eg, industrial surveys), calibration checking and quality control procedures should be repeated prior to initiating further testing.

V. MANEUVER PERFORMANCE RECOMMENDATIONS

Personnel Qualifications

The ATS has made recommendations for laboratory personnel performing a variety of pulmonary function testing tasks [41]. In addition to at least a high school training background, strong mathematics training is encouraged. Also, 1 or more years of college or equivalent training are preferred for technicians performing spirometry. For pulmonary function laboratories, 6 months of supervised training time is recommended for performing spirometry. If troubleshooting is to be a part of the laboratory technician's responsibility, a training period of 1 year is recommended. The ATS has taken a strong position that Medical Directors must have appropriate training and be responsible for all pulmonary function testing [42]. Training for doing epidemiological spirometric testing may be more intensive than that of a technician for a general pulmonary laboratory testing and may thus be

accomplished more quickly. For industrial/occupational testing, there are training requirements mandated by the National Institute for Occupational Safety and Health (NIOSH) [18] and industry [33] and the ACCP [43].

Several excellent training manuals have been prepared for performance of spirometry [17,18,33,44] and NIOSH approves training courses [18].

Rationale. The testing of equipment and wide-scale proficiency testing of pulmonary function equipment is not currently feasible. However, using laboratory personnel as "known subjects" and performing intra-laboratory and inter-laboratory testing can be helpful [38]. In addition, the ATS has recently published guidelines for "Quality Assurance in Pulmonary Function Laboratories" [38], which are recommended.

With the decrease in size and cost of microprocessors and the increase in their speed and reliability, most spirometer systems will contain some type of digital computer. Indeed, in a recent test of 53 commercially available spirometers only 3 did not contain a computer [6]. New quality assurance problems will occur as pulmonary function laboratories become more reliant on digital computers and associated automation [45,46].

The use of computers to perform spirometry has accelerated in the past five years, and this trend may be advantageous to obtain accurate spirometry [5,35]. The recent testing of commercially available spirometers showed that a major source of errors was in computer software [6]. Because of the increased use of computers in pulmonary laboratories and the problems associated with them [6,45], the ATS has published "Computer Guidelines for Pulmonary Laboratories" [46], which should be followed.

Recommendation—FVC Subject Instruction and Maneuver

Subjects will be instructed in the FVC maneuver, and the appropriate technique will be *demonstrated*. A *minimum* of 3 acceptable FVC maneuvers will be performed. If a subject has large variability between expiratory maneuvers, reproducibility criteria may require that up to 8 acceptable maneuvers be performed. See Figure 3 and Section VII for further clarification.

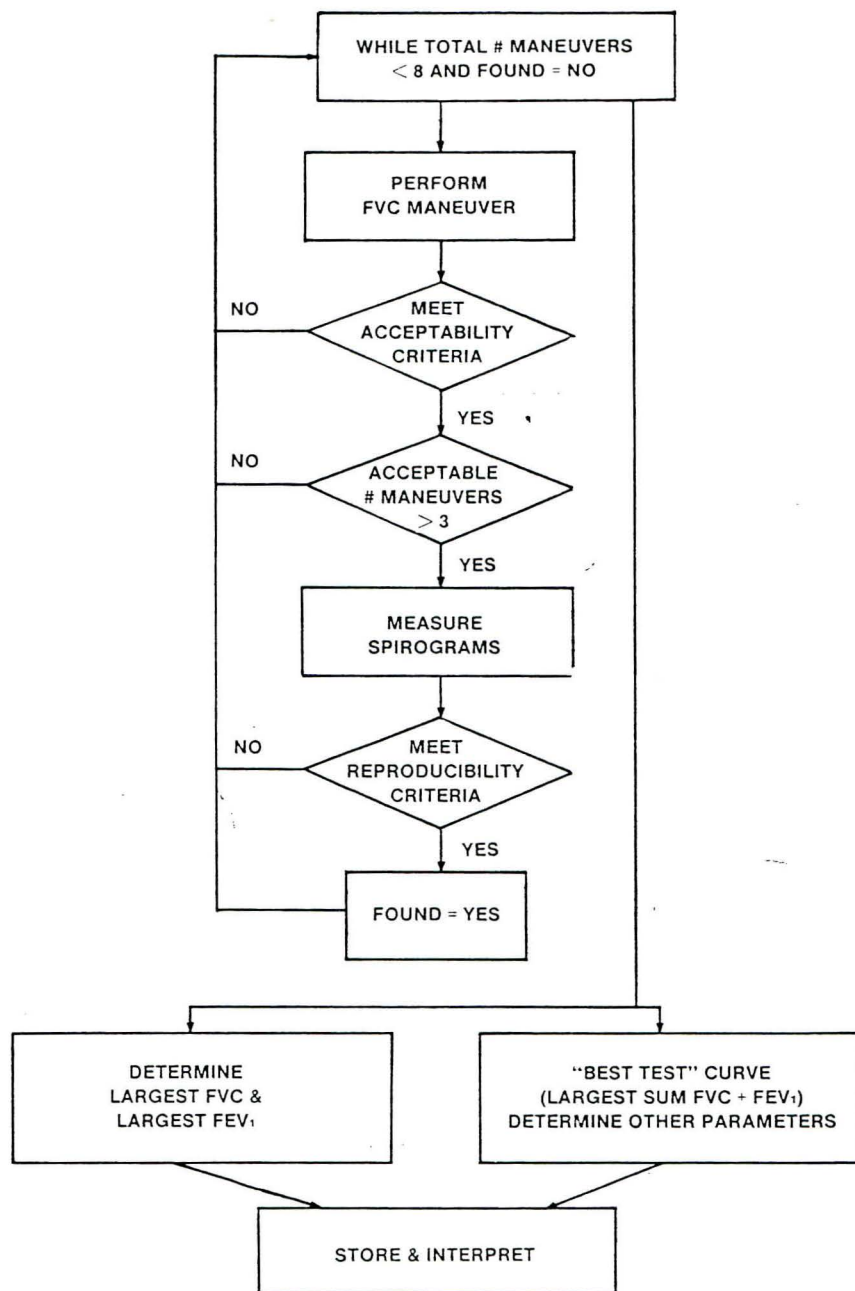


Fig. 3. Flow chart diagram of FVC spirometry testing

Recommendation—FVC End-of-Test Criteria

Subjects should be verbally exhorted to continue to squeeze out the air at the end of the maneuver. "End of Test" will occur when there is: (1) an obvious plateau in the volume-time curve resulting in no

change in volume for *at least 2 s* (a volume decrease is, for the purposes of end-of-test selection, equivalent to no change in volume) with an exhalation time of *at least 6 s* (longer times are frequently needed for subjects with airway obstruction). For the purposes of this criterion, no change in volume is the minimal detectable volume of the spirometer. Minimum detectable

volume *must be at least 0.040 L*; or (2) a forced exhalation of reasonable duration. (For example, exhalation times of greater than 15 s in subjects with severe airway obstruction will rarely change clinical decisions and longer exhalations are seldom justified. Manufacturers should note, however, that several of the 24 test waveforms have durations longer than 20 s); or (3) when, for legitimate clinical reasons, the subject cannot or should not continue further exhalation.

Although the end-of-test criteria defined above are reasonable and will perform adequately in most situations, spirometers should not prevent the continued accumulation of volume after the end-of-test criteria are met. We encourage spirometer designs that allow technicians to encourage subjects to breathe out for as long as they can or until there is an inspiration.

Rationale. A recent study [19] using standard waveforms has shown that application of the earlier ATS recommended "end of test" criteria [1] prematurely terminates the FVC maneuver, resulting in as much as a 9% reduction in the measured FVC. Because the original recommendation was not based on data from subjects who covered the full spectrum of the population, the end-of-test criteria are now being updated.

Requiring that there be no change in volume for at least 2 s is probably similar to long-standing manual methods. We were reluctant to use the minimum volume accuracy of 0.050 L for the minimum detectable volume because most spirometers can resolve volume less than 0.050 L. Manual spirometers with a strip chart recorder can typically resolve 0.025 L, and a spirometer with a digital shaft encoder can typically resolve a 0.010-L volume [47]. The second end-of-test criterion (*reasonable duration of 15 s*) is necessary to avoid prolonged expirations in subjects with severe airway obstruction in whom more prolonged expiratory efforts will not change the clinical decision.

Recommendation—Minimum FVC Exhalation Time

A minimum exhalation time of 6 s, unless there is an obvious plateau, is required to obtain maximal FVC results. Longer times

are often required to achieve "end of test," particularly in obstructed individuals.

Recommendation—FVC Satisfactory Start-of-Test Criteria

To achieve accurate "time zero" and ensure that the FEV₁ comes from a maximal effort curve, the extrapolated volume should be less than 5% of the FVC or 0.100 L, whichever is greater. See Figure 2 for example of back extrapolation.

Rationale. The allowable extrapolated volume of the current ATS recommendations was 10% of the FVC or 0.100 L, whichever was greater, which can result in very slow starts with low peak flows being acceptable [1,48-50]. In addition, FEV₁ from submaximal efforts can be larger than those obtained when a maximal effort is performed, both due to a volume of air being exhaled without being timed (the extrapolated volume) and to less dynamic compression of airways in some subjects with submaximal efforts. Because the largest FEV₁ is reported, a falsely elevated FEV₁ may be used in the final report. The lower allowable extrapolated volume should reduce the effect of submaximal effect on the reported FEV₁.

Recommendation—FVC Maximum Number of Maneuvers

Although there may be some circumstances in which more than 8 consecutive FVC maneuvers are needed, 8 maneuvers is considered a practical upper limit for most subjects.

Rationale. After several forced expiratory maneuvers, fatigue begins to take its toll on subjects and, thus, their spirometric parameters. In addition, some subjects may exhibit spirometry-induced bronchospasm, and additional maneuvers would be of little added value. Therefore, an upper limit of the number of maneuvers is warranted. Ferris and associates [51] and Kanner and colleagues [15] have reported that for adults and children 8 maneuvers is a practical upper limit.

Recommendation—FVC Environmental Conditions

Spirometric testing with ambient temperatures less than 17° C or above 40°

C is not recommended. Ambient temperature should *always* be recorded and reported to an accuracy of $\pm 1^\circ$ C. Spirometer users should be aware of the problems with testing done at lower temperatures. Ranges of barometric pressures that are acceptable for the spirometer should be published by the manufacturer.

Rationale. There is evidence that some subjects may develop airflow limitation with the inhalation of very cold air. Therefore, spirometry should not be conducted when the ambient temperature is cold enough to induce airflow limitation.

Recent studies also point out the problem of finite cooling times of gases in volume-type spirometers and their associated tubing [52-54]. In one of these studies, it was found that a +7.7 to 14% error of FEV₁ results if the volume-type spirometer is at an ambient temperature of 3° C, even with the BTPS correction. This error is less if the spirometer is warmer (nearer body temperature) [52]. As a result, 17° C was judged to be an acceptable and reasonable lower limit.

Complexities related to temperature are also encountered with flow-measuring devices [54-57]. Air exhaled from the mouth is estimated to be at 33° C [55,56]. If any connecting tubing is used between the mouthpiece and the flow sensor, the exhaled gas will experience a variable amount of cooling if the room temperature is not at 33° C. Details of the cooling pattern for flow spirometers have not been studied, but they may result in errors similar to those for volume devices [54-58].

Because not all spirometers are used at sea level ($P_B = 760$ mm Hg), the range of barometric pressures allowed by the spirometer and its associated computational equipment should be specified.

Recommendation—FVC Use of Nose Clips

Use of nose clips is encouraged.

Rationale. Although the use of nose clips does not appreciably influence the FVC performed using the open-circuit technique, some subjects breathe through the nose during the maneuver when closed circuit technique is used.

Recommendation—FVC Sitting versus Standing

Subjects may be studied in the sitting or standing position. Indication of position is necessary.

Rationale. Recent studies by Townsend show that for adults there are significantly larger forced expiratory volumes in the standing position than in the sitting position [59]. The earlier ATS recommendation indicates that in children, VC is greater in the standing than in the sitting position [1].

VI. MEASUREMENT PROCEDURES

Measurement

Spirometric variables should be measured from a series of *at least* 3 acceptable forced expiratory curves.

Rationale. Best efforts cannot always be determined by simple inspection of a spirogram. Measurements and calculation are required to determine the largest values.

Recommendation—Test Result Selection/Reporting of Results

The largest FVC and the largest FEV₁ (BTPS) should be recorded, after examination of the data from all the acceptable curves, *even if the two values do not come from the same curve.* Other measures such as the FEF_{25-75%} and/or the instantaneous expiratory flows (\dot{V}) should be obtained from the single "best test" curve [1,17]. The best-test curve is defined as the test that meets the acceptability criteria and gives the largest sum of FVC plus FEV₁.

Rationale. Two competing methods for selection of FVC and FEV₁ values have been used: (1) using the largest FVC and the largest FEV₁ independent of which acceptable curve they came from; or (2) using the FVC and FEV₁ from the single best-test curve with the largest sum of FVC plus FEV₁.

As a result of the original recommendations made by the ATS Snowbird Workshop, several investigators have evaluated the use of the best-test method [60-62]. The University of Arizona group used the single best test to reevaluate their data and found that construction of

"composite" maximal expiratory flow-volume (MEFV) curves gave results that were systematically higher than taking data from a best-test waveform [60,61]. Sorensen and associates demonstrated that differences between maximal and best-test FVC and FEV₁ were small. The mean difference between the 2-test result selection methods was only 5.8 ml for FVC and 8.4 ml for FEV₁. In 98.4% of the FVC comparisons and 95.7% of the FEV₁ comparisons, the differences were within the minimal spirometer accuracy recommendations (± 0.050 L or $\pm 3\%$ of reading) [62].

The Committee decided to continue with the original Snowbird recommendation of taking the largest FVC and the largest FEV₁ independent of which curve they came from, for the following reasons: (1) A large base of data, especially from epidemiological studies, has been collected with the current recommended methods, and, because the differences between "largest" and "best test" were small, no change in the recommendation was justified. (2) The FVC and FEV₁ are independent and therefore may be selected from different curves. (3) The largest values represent a subject's highest potential values and therefore should be used for legal/regulatory purposes. In fact, these regulations are already in place and will not likely change.

The Committee decided to continue with the original Snowbird recommendation of taking the largest FVC and the largest FEV₁ independent of which curve they came from, for the following reasons: (1) A large base of data, especially from epidemiological studies, has been collected with the current recommended methods, and, because the differences between "largest" and "best test" were small, no change in the recommendation was justified. (2) The FVC and FEV₁ are independent and therefore may be selected from different curves. (3) The largest values represent a subject's highest potential values and therefore should be used for legal/regulatory purposes. In fact, these regulations are already in place and will not likely change.

Because the average differences between the two methods are so small (< 10 ml), any reference-value studies [63] or epidemiological studies previously done with the best-test method are still valid.

VII. ACCEPTABILITY AND REPRODUCIBILITY

Recommendation—FVC Maneuver Acceptability

Acceptability will be determined by ascertaining that the recommendations outlined above in the section on performing the FVC test are met. In review these are: (1) end-of-test criteria, (2) minimum FVC exhalation time of 6 seconds, and (3) satisfactory start of test. In addition the technician should observe that the subject understood the instructions and performed the maneuver with a maximum inspiration, with a good start, with a smooth continuous exhalation, with maximal effort, and without:

- (1) An unsatisfactory start of expiration, characterized by excessive hesitation or false start or extrapolated volume of greater than 5% of FVC or 0.100 L, whichever is greater.
- (2) Coughing during the first second of the maneuver (thereby affecting the measured FEV₁ value) or any other cough that in the technician's judgment interferes with measurement of accurate results.
- (3) Valsalva maneuver (glottis closure).
- (4) Early termination of expiration. (In a *normal* subject this would be before completion of the breath—*usually* less than a 6-s maneuver. In an obstructed subject a longer time is required [64,65].)
- (5) A leak.
- (6) An obstructed mouth piece, eg, obstruction due to the tongue being placed in front of the mouthpiece, false teeth falling in front of the mouthpiece, etc.

Figure 3 is a flow chart outlining how acceptability and reproducibility criteria are to be applied.

Rationale. Many patients cough and sputter toward the end of their FVC maneuver, but this does not affect the important initial spirometry parameters. To eliminate these FVC maneuvers from clinical evaluation would be a waste of useful information. *At least* 3 acceptable maneuvers are required to ensure that maximal effort and cooperation are obtained and that the resulting data provide an accurate reflection of the subject's pulmonary function [1]. This conclusion was achieved after review of the data of Knudson and associates [66] and others [17,67].

Recent studies [48-50] have shown that the elimination of subjects for failure to meet the ATS reproducibility criteria may result in elimination of data from subjects who have abnormal lung function, resulting in a population bias. Pennock et al [68] have reported that subjects with obstruction have greater coefficients of variation than do normal subjects. Therefore, these subjects are more likely to be unable to meet the ATS minimum-reproducibility criteria. The reproducibility criteria have been clarified to eliminate confusion. If acceptability criteria are not applied before the reproducibility criteria, then a passive exhalation maneuver will often be labeled as the "best" maneuver because it may give the largest sum of FVC + FEV₁.

Recommendation—FVC Test-Result Reproducibility

As a goal during test-result performance, the largest FVC and second largest FVC from acceptable curves should **not** vary by more than 5% of reading (expressed as a percentage of the largest observed FVC regardless of the curve on which it occurred) or 0.100 L, whichever is greater. In addition to the FVC criteria, the largest FEV₁ and the second largest FEV₁ (expressed as a percentage of the largest observed FEV₁ regardless of the curve on which it occurred) should not vary by more than 5% of reading or 0.100 L, whichever is greater.

The reproducibility criteria are used as a guide to whether more than 3 FVC maneuvers are needed; these criteria are **not** to be used for excluding results from reports or for excluding subjects from a study. Labeling results as being derived from data that do not conform to the reproducibility criteria stated above is encouraged (especially when the data suggest that bronchospasm was triggered by the FVC maneuver). The acceptability criteria should be applied before the reproducibility criteria (See Figure 3). Unacceptable maneuvers should be discarded before applying the reproducibility criteria.

The only criterion for unacceptable subject performance requiring elimination from further consideration is less than 2 acceptable curves. No spirogram should be

rejected solely on the basis of its poor reproducibility, provided 3 acceptable maneuvers were obtained. Reproducibility of results should be considered at the time of interpretation. Use of data from maneuvers with poor reproducibility is left to the discretion of the interpreter.

Rationale. It was not clear from the earlier ATS statement on standardization of spirometry whether the 5% referred to FVC, FEV₁, or both FVC and FEV₁. Recent studies [48-50] have shown that the elimination of subjects for poor reproducibility may inappropriately eliminate subjects, resulting in a population bias. Pennock and associates have reported that subjects with airway obstruction have greater coefficients of variation than normal subjects [68]. Therefore, these subjects are more likely to be unable to meet the initial ATS minimum-reproducibility criteria. In addition, the reproducibility should be changed to eliminate any confusion concerning which values are used and when the reproducibility criteria are applied. If acceptability criteria are not applied before the reproducibility criteria, then a passive exhalation maneuver may be labelled as the "best" maneuver if it gives the largest sum of FVC + FEV₁.

The calculation of the FVC and FEV₁ reproducibility presents no problem for a computer; however, the need for rapid determination of FEV₁ during the testing session presents a recognized logistics problem if results are hand measured and calculated.

VIII. REFERENCE VALUES AND INTERPRETATION STANDARDIZATION

This area of spirometry standardization is at an early stage in its development. The Intermountain Thoracic Society has recently published its Manual of Uniform Laboratory Procedures [17]. The California Thoracic Society has published a similar book, which emphasized the controversy associated with selecting reference values and interpretation methodology [69].

Reference-value determination is clearly an area of spirometry that must be further investigated and standardized. There are well over 20 reference-value equations for spirometry in common use. Few data are available for several race and age groups.

Although it is too early to standardize reference values, the committee recommends that, as a minimum, reference values for FVC and FEV₁ come from the same study so that they are internally consistent.

The standardization of interpretive procedures is also in need of further investigation [70]. The present situation allows enough interpretive variability to cause identical data from a patient to be interpreted differently in different laboratories [71].

IX. CLINICAL ASSESSMENT

Clinical/Epidemiologic Considerations

Whether the spirogram results are to be used for clinical or epidemiological purposes, the above recommendations apply.

Classification

The classification of spirometry into normal and abnormal groupings and into disease categories such as mild, moderate, and severe airway obstruction is simple and is easily performed by a computer once criteria have been established. The meaning of such classifications requires clinical information. For example, the meaning of an FVC measurement that is just below the lower limit of normal is different in a young, healthy, non-smoking individual than it is in a person who presents for evaluation of dyspnea or who has an abnormal chest radiograph. In the first case, the probability of a false-positive test is large because the prior probability of disease is very low. In the second case, the probability of a true-positive test is high because the symptoms and/or the abnormal radiograph increase the prior probability of disease. One area that causes considerable controversy is the combined obstruction and restriction classification. This classification is commonly made when airway obstruction is present. The problem is that the FVC is reduced out of proportion to what was expected from the degree of obstruction. This problem may be more easily resolved when absolute lung volumes are available and when it is approached in the context of the patient's clinical problems

and when other clinical information such as a chest radiograph is available.

Committee on Proficiency
Standards for Clinical
Pulmonary Function
Laboratories

Reed M Gardner PhD, Chairman
John L Hankinson PhD
Jack L Clausen MD
Robert O Crapo MD
Robert L Johnson Jr MD
Gary R Epler MD

ACKNOWLEDGMENTS

The Committee thanks those who have provided input to this update of the Standardization of Spirometry. Special thanks goes to original participants of the Snowbird Workshop whose valued input was sought and used. Steven B Nelson provided valuable input on testing methods. Results from his research on validating spirometers gave us insight into how to perform the testing and what were reasonable and fair expectations of contemporary spirometers [6]. Steven L Berlin provided support with waveform graphics.

External reviewers Drs Paul L Enright, Millicent W Higgins, Henry W Glindmeyer, and Edward P Horvath Jr provided excellent suggestions. The following American Lung Association Committee on Occupational Health members provided wisdom and careful reviews: Drs David W Cugell, Robert M Castellani, and Benjamin G Ferris Jr. Finally, Dr A Sonia Buist of the ATS Board of Directors gave essential input and was an enthusiastic supporter.

REFERENCES

1. American Thoracic Society Statement: Standardization of spirometry. *Am Rev Respir Dis* 1979;119:831-838.
2. Zamel N, Altose MD, Speir WA Jr. ACCP Scientific Section Recommendations. Statement of spirometry: A report of the section on respiratory pathophysiology. *Chest* 1983;83:547-550.
3. Taussig LM, Chernick V, Wood R, Farrell P, Mellins RC. Conference Committee. Standardization of lung function testing in children. *J Pediatr* 1980;97:668-678.
4. Quanjer PH, editor. Standardization of lung function testing. *Bull Eur Physio-pathol Respir* 1983;19(5,suppl).

5. Renzetti AD Jr, Bleecker ER, Epler GR, Jones RN, Kanner RE, Repsher LH. Evaluation of impairment/disability secondary to respiratory disorders. *Am Rev Resp Dis* 1986;133:1205-1209.
6. Nelson SB. Commercially available spirometers: Performance evaluation. MS Thesis, Department of Medical Informatics, University of Utah 1987.
7. Hankinson JL. Pulmonary function testing in the screening of workers: Guidelines for instrumentation, performance, and interpretation. *J Occup Med* 1986;28:1081-1092.
8. Pulmonary terms and symbols: A report of the ACCP-ATS Joint Committee on Pulmonary Nomenclature. *Chest* 1975;67:583.
9. Hankinson JL, Petersen MR. Data analysis for spirometry instrumentation standards (abstract). *Am Rev Respir Dis* 1977;115 (5, Part 2:116).
10. Dickman ML, Schmidt CD, Gardner RM. Spirometric standards for normal children and adolescents (ages 5 years through 18 years). *Am Rev Respir Dis* 1971;104:680-687.
11. Knudson RJ, Slatin RC, Lebowitz MD, Burrows B. The maximum expiratory flow volume curve: Normal standards, variability and effects of age. *Am Rev Respir Dis* 1976;113:587.
12. Schmidt CD, Dickman ML, Gardner RM, Brough FK. Spirometric standards for healthy elderly men and women. *Am Rev Respir Dis* 1973;108:933-939.
13. Glindmeyer HW. An experimental investigation of the errors of spirometry. PhD thesis, Tulane University, New Orleans LA, 1976.
14. Glindmeyer HW III, Anderson ST, Diem JF, Weill H. A comparison of the Jones and Stead-Wells spirometers. *Chest* 1978;73:596.
15. Kanner RE, Schenker MB, Munoz A, Speizer FE. Spirometry in children: Methodology for obtaining optimal results for clinical and epidemiological studies. *Am Rev Respir Dis* 1983;127:720-724.
16. Smith AA, Gaensler EA. Timing of forced expiratory volume in one second. *Am Rev Respir Dis* 1975;112:882.
17. Morris AH, Kanner RE, Crapo RO, Gardner RM. Clinical pulmonary function testing: A manual of uniform laboratory procedures, 2nd ed. July 1984.
18. Horvath EP Jr, ed. Manual of spirometry in occupational medicine. Division of Training and Manpower Development, National Institutes for Occupational Safety and Health. Nov 1981. NIOSH. Robert Taft Bldg, 4676 Columbia Parkway, Cincinnati Ohio 45226.
19. Hankinson JL, Gardner RM. Standard waveforms for spirometer testing. *Am Rev Respir Dis* 1982;126:362-364.
20. Knudson R, Lebowitz MD, Slatin RC. The timing of the forced vital capacity. *Am Rev Respir Dis* 1979; 119:315-318.
21. Federal Register 38:4265, Feb 12, 1973, Section of pulmonary function specifications.
22. Cotes JE. Assessment of mechanical attributes. In: Lung function; Assessment and application in medicine, 2nd ed. Oxford: Blackwell Scientific Publications, 1968:96.
23. Shepherd RJ. Some observations of peak expiratory flow. *Thorax* 1962;17:39.
24. Respiratory function tests in pneumoconiosis. Occupational Safety and Health Series #6. Geneva, Switzerland: International Labor Organization, 1966.
25. Gaensler EA. Analysis of the ventilatory defect by timed capacity measurements. *Am Rev Tuberc* 1951;64:256.
26. Gaensler EA. An instrument for dynamic vital capacity measurements. *Science* 1951;114:444.
27. Cochrane GM, Prieto F, Clark TJH. Intrasubject variabilities of maximum expiratory flow volume curve. *Thorax* 1977;32:171.
28. McCall CB, Hyatt RE, Noble FW, Fry DL. Harmonic content of certain respiratory flow phenomena in normal individuals. *J Appl Physiol* 1957;10:215.
29. Gaensler EA, Rayl DF, Donnely DM. The breath holding test in pulmonary insufficiency. *Surg Gynecol Obstet* 1951;92:81.
30. Bartlett RG Jr, Bruback H, Specht H. Some factors determining the maximum breathing capacity. *J Appl Physiol* 1958;12:247.
31. Swi S, Theron JC, McGregor M, Becklake MR. The influence of instrumental resistance on the maximum breathing capacity. *Dis Chest* 1959;36:361.
32. Baldwin F, Courmand A, Richards DW Jr. Pulmonary insufficiency. I. Physiological classification, clinical methods of analysis, standards values in normal subjects. *Medicine* 1948;27:243.
33. Pulmonary Function Standards for Cotton Dust. 29 Code of Federal Regulations;1910.1043 Cotton Dust, Appendix D. Occupational Safety and Health Administration 1980;808-832.
34. Morgan KC, chairman (Committee Recommendations) The assessment of ventilatory capacity. *Chest* 1975;67:95.
35. Gardner RM, Crapo RO, Billings RG, Shigeoka JW, Hankinson JL. Spirometry: What paper speed? *Chest* 1983;84:161-165.
36. Association for the Advancement of Medical Instrumentation. Standard for spirometers (draft). October 1980. AAMI Suite 602, 1901 N Ft Myer Drive, Arlington VA 22209-1699
37. Gardner RM, Hankinson JL, West BJ. Evaluating commercially available spirometers. *Am Rev Respir Dis* 1980;121:73-82.
38. Gardner RM, Clausen JL, Crapo RO, Epler GR, Hankinson JL, Johnson RL Jr, Plummer AL. Quality assurance in pulmonary function laboratories. *Am Rev Respir Dis* 1986;134:626-627.
39. Tablan OC, Williams WW, Martone WJ. Infection control in pulmonary function laboratories. *Infect Control* 1985;6:442-444.
40. Townsend MC. The effects of leaks in spirometers on measurement of pulmonary function. *J Occup Med* 1984;26:835-841.
41. Gardner RM, Clausen JL, Epler G, Hankinson JL, Permutt S, Plummer AL. Pulmonary function laboratory personnel qualifications. *Am Rev Respir Dis* 1986;134:623-624.
42. George RB et al. ATS Respiratory Care Committee—Position paper: Director of pulmonary function laboratory. *ATS News* 1978;4:6.
43. Make B. Minimum criteria for training course in spirometric testing in industry. *Bull Am Coll Chest Phys* 1979;18:24-26.
44. Enright PL, Hyatt RD. Office spirometry. Philadelphia: Lea & Febiger Publishers, 1987.
45. Crapo RO, Gardner RM, Berlin SL, Morris AH. Automation of pulmonary function equipment—User beware! (editorial) *Chest* 1986;90:1-2.
46. Gardner RM, Clausen JL, Cotton DJ, Crapo RO, Epler GR, Hankinson JL, Johnson RL Jr. Computer guidelines for pulmonary laboratories. *Am Rev Respir Dis* 1986;134:628-629.
47. Ostler DV, Gardner RM, Crapo RO. A computer system for analysis and transmission of spirometry waveforms using volume sampling. *Comput Biomed Res* 1984;17:229-240.
48. Eisen EA, Robins JM, Greaves IA, Wegman DH. Selection: Effects of repeat ability criteria applied to lung spirometry. *Am J Epidemiol* 1984;120:734.
49. Eisen EA, Oliver LC, Christiani DC, Robins JM, Wegman DH. Effects of spirometry standards in two occupational cohorts. *Am Rev Respir Dis* 1985;132:120.
50. Kellie SE, Attfield MD, Hankinson JL, Castellan RM. The ATS spirometry variability criteria: Associations with morbidity and mortality in an occupational cohort of coal miners. *Am J Epidemiol* 1987;125:437-444.

51. Ferris BG Jr, Speizer FE, Bishop Y, Prang G, Weener J. Spirometry for an epidemiologic study: Deriving optimum summary statistics for each subject. *Bull Eur Physiopathol Respir* 1978;14:146-166.
52. Hankinson JL, Viola JO. Dynamic BTPS correction factors for spirometric data. *J Appl Physiol: Respirat Environ Exercise Physiol* 1983;44:1354.
53. Hankinson JL, Castellano RM, Kinsley KB, Keimig DG. Effects of spirometer temperature on FEV₁ shift changes. *J Occup Med* 1986;28:1222-1225.
54. Pincock AC, Miller MR. The effect of temperature on recording spiograms. *Am Rev Respir Dis* 1983;128:894-898.
55. Miller MR, Pincock AC. Linearity and temperature control of the Fleisch pneumotachograph. *J Appl Physiol* 1986;60:710-715.
56. Cole P. Recordings of respiratory air temperature. *J Laryngol* 1954;68:295-307.
57. Liese W, Warwick WJ, Cumming G. Water vapour pressure in expired air. *Respiration* 1974;31:252-261.
58. Perks WH, Sopwith T, Brown D, Jones CH, Green M. Effects of temperature on Vitalograph spirometer readings. *Thorax* 1983;38:592-594.
59. Townsend MC. Spirometric forced expiratory volumes measured in the standing versus the sitting posture. *Am Rev Respir Dis* 1984;130:123-124.
60. Nathan SP, Lebowitz MD, Knudson RJ. Spirometric testing: Number of tests required and selection of data. *Chest* 1970;76:384-388.
61. Knudson RJ, Lebowitz MD, Holberg CJ, Burrows B. Changes in the normal maximal expiratory flow-volume curve with growth and aging. *Am Rev Respir Dis* 1983;127:725-734.
62. Sorensen JB, Morris AH, Crapo RO, Gardner RM. Selection of the best spirometric values for interpretation. *Am Rev Respir Dis* 1980;122:802-805.
63. Crapo RO, Morris AH, Gardner RM. Reference spirometric values for spirometry using techniques and equipment that meet ATS recommendations. *Am Rev Respir Dis* 1981;123:659-664.
64. Ferris BG. Epidemiology standardization project: Recommended standardized procedures for pulmonary function testing. *Am Rev Respir Dis* 1978;118:(Part 2).
65. Townsend MC, DuChene AG, Fallat RJ. The effects of underrecording forced expirations on spirometric lung function indexes. *Am Rev Respir Dis* 1982;126:734-737.
66. Knudson RJ, Burrows B, Lebowitz MD. The maximal expiratory flow volume curve: Its use in the detection of ventilatory abnormalities in a population study. *Am Rev Respir Dis* 1976;111:871.
67. Tager I, Speizer FE, Rosner B, Prang G. A comparison between the three largest and three last of five forced expiratory maneuvers in a population study. *Am Rev Respir Dis* 1976;114:1201.
68. Pennock BE, Rogers RM, McCaffree DR. Changes in measured spirometric indices: What is significant? *Chest* 1981;80:97.
69. Clausen JL, Zarins LP, eds. Pulmonary function testing: Guidelines and controversies. New York: Academic Press 1982.
70. Leiner GC, Abramowitz S, Small MJ. Pulmonary function testing in laboratories associated with residency training programs in pulmonary disease. *Am Rev Respir Dis* 1968;100:240-244.
71. Clausen JL, Crapo RO, Gardner RM. Interlaboratory comparisons of pulmonary function testing (abstract). *Am Rev Respir Dis* 1984;129:A37.
72. Lemen RJ, Gerdes CB, Wegmann MJ, Perrin KJ. Frequency spectra of flow and volume events for forced vital capacity. *J Appl Physiol* 1982;53:977-984.
73. Jerri AJ. The Shannon sampling theorem: Its various extensions and applications—A tutorial review. *Proc IEEE* 1977;65:1565-1596.
74. Lanczos C. *Applied Analysis*. Englewood Cliffs: Prentice-Hall, 1956:321-324.